Chlorine Dioxide

CIO2 3E 1 O (unfiltered)

CIO2 3E 1 O

FEATURES

Amperometric 3 electrode sensor cell Low susceptibility to abrupt changes of humidity Interference to Chlorine High selectivity 0 voltage biased operation

TYPICAL APPLICATIONS

Pulp & Paper Industry, Water treatment plants, Desinfection Portable and fixed point monitoring of TLV levels

PART NUMBER INFORMATION

MINI	2731-331-30009
4 series adaptation	2731-331-30049
7 series adaptation	2731-331-30079

Note:

It is recommended to cross calibrate with 1 –5 ppm chlorine

CIO2 3E 1 O

TECHNICAL SPECIFICATIONS

Measuring Range 0–1 ppm

Sensitivity Range 600 nA/ppm ± 200 nA/ppm (negative signal)

Zero Current at $20 \,^{\circ}\text{C}$ $< \pm 15 \,\text{nA}$ Resolution at $20 \,^{\circ}\text{C}$ $< 0.03 \,\text{ppm}$ Bias Potential $0 \,\text{mV}$

Linearity < 10% full scale

Response Time at 20 ℃

t50 < 20 s calculated from 4 min. exposure time

t90 < 120 s (typically < 60 s), calculated from 4 min. exposure

Long Term Sensitivity Drift <10% per 6 months

Operation Conditions

Temperature Range -20 °C to +40 °C

Humidity Range 15–90% r.H, non-condensing


Effect of Humidity no effect

Sensor Life Expectancy > 24 months in air

Warranty 12 months


CIO2 3E 1 O

OUTPUT vs. TEMPERATURE: (calibration has been done using 1 ppm Cl2 instead of ClO2)

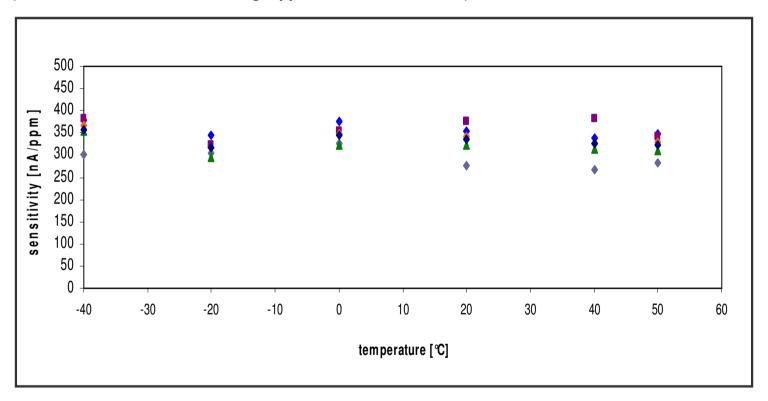

CIO2 3E 1 O

ZERO READING vs. TEMPERATURE: (calibration has been done using 1 ppm Cl2 instead of ClO2)

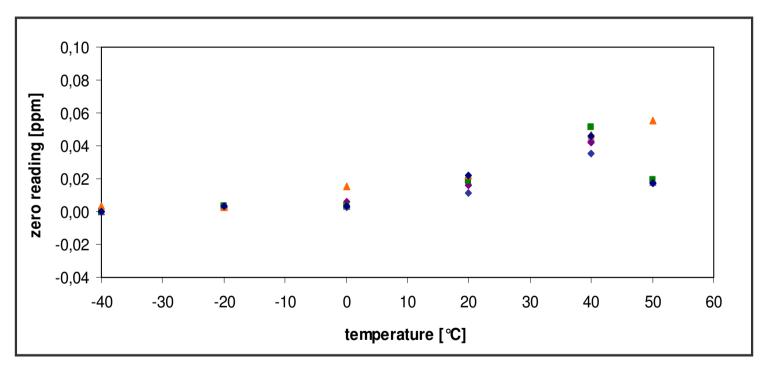

CIO2 3E 1 O

CROSS SENSITIVITIES AT 20 ℃

Gas	Concentration	Reading [ppm]
Alcohols	1000 ppm	0
Carbon Monoxide	100 ppm	0
Chlorine	1 ppm	0.6
Ozone	0.25 ppm	0.7
Hydrogen	3000 ppm	0
Hydrogen Sulfide	20 ppm	-5

Notes:

- 1. Interference factors may differ from sensor to sensor and with life time.
- 2. This table does not claim to be complete. The sensor might also be sensitive to other gases.
- 3. It is recommended to use 1-5 ppm Cl_2 for cross calibration.

Safety Note

This sensor is designed to be used in safety critical applications. To ensure that the sensor and/or instrument in which it is used, are operating properly, it is a requirement that the function of the device is confirmed by exposure to target gas (bump check) before each use of the sensor and/or instrument. Failure to carry out such tests may jeopardize the safety of people and property.

Attention

Use of this range of sensors requires complete understanding of the instructions. Before using this range sensors please carefully read 'Application Notes'.

For further assistance on sensor selection and use, please contact a member of the Technical Sales team.